




Operating Instructions

Temperature Controller

type 201

(APPLICABLE WHEN ALARM FEATURE IS IN USE)

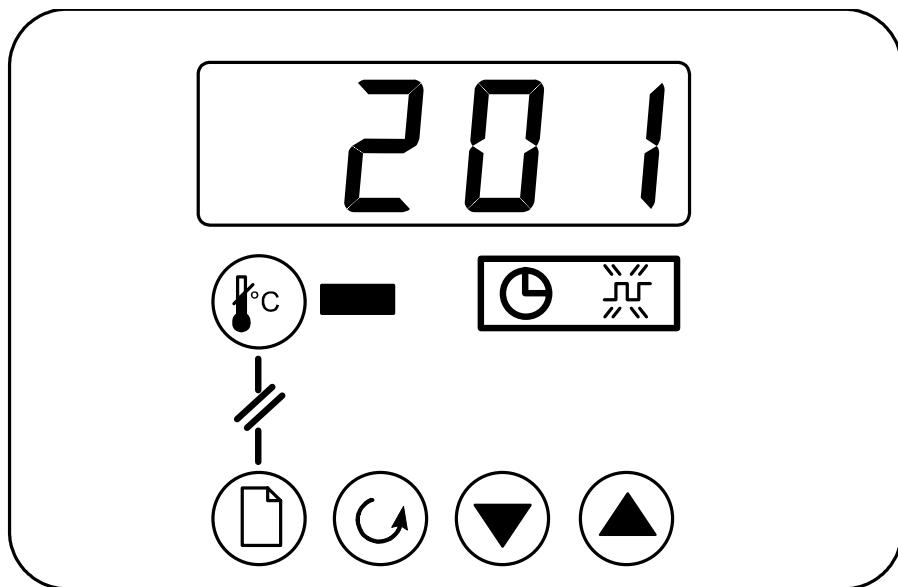

CONTENTS

section	page
1 Description	1
2 Basic Operating Instructions	3
3 Overtemperature Option	5
4 Altering the Power Limit	5
5 User Calibration	6
6 Navigation Diagrams	7

See also the main manual for the furnace, oven or other product to which the controller is fitted.

DESCRIPTION

1.1 201 Controller

The model 201 controller is made especially for Carbolite by Eurotherm, and shares many of the features of the Eurotherm 2000 range, especially the model 2132. It is a digital instrument with PID control algorithms. It is supplied as an integrated part of the control section of the oven or furnace.

The 201 features:

- Easy use as a simple temperature controller, where on setting the required temperature the controller immediately attempts to reach and maintain it.
- A ramp-to-setpoint feature, which may be used to limit the heating (or cooling).
- An alarm output which may be used in conjunction with a solid state relay for miscellaneous control purposes.

The controller does not contain a real-time calendar, and is not subject to century-end date problems.

1.2 Model 201 Overtemperature Controller

The 201 is optionally available as a dual unit containing the main controller and an overttemperature controller. These two components share the same display and buttons, but are otherwise independent.

The operational features in the overttemperature controller include:

- Easy setting of the overttemperature limit (setpoint);
- A visible alarm on overttemperature condition;
- A latching alarm output used to cut power to the heating elements; this alarm output can also be used to power an optional audible alarm;
- 2-key alarm acknowledgement.


BASIC OPERATING INSTRUCTIONS

2.1 Furnace or Oven Controls

Most Carbolite products are fitted with an “Instrument Switch” which cuts off power to the controller and other parts of the control circuit. See the instruction manual for the furnace or oven for the overall operating instructions.

To operate the 201 there must be power to the furnace or oven, and the Instrument switch must be on. If a time switch is included in the furnace or oven circuit, this must be in an On period.

2.2 The 201 – Operation

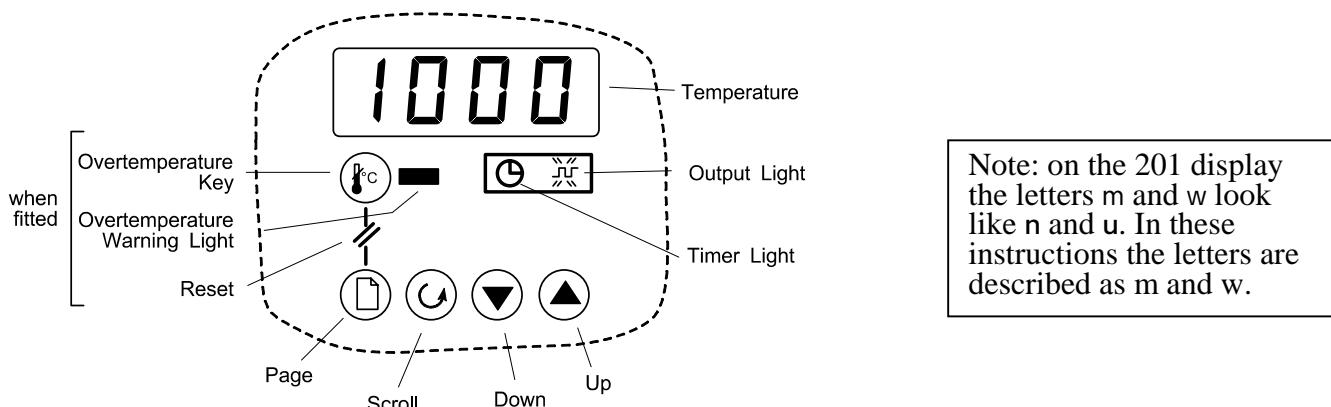

When switched on, the controller lights up, goes through a short test routine, and then displays the measured temperature and starts to control. The output light glows or flashes as heating occurs.

The **Page** key allows access to parameter lists within the controller; most lists and parameters are hidden and cannot be accessed by the operator because they contain factory-set parameters which should not be changed.

A single press of the page key displays the temperature units, normally set to °C; further presses reveal the lists indicated in the Navigation Diagram in section 6.

The **Scroll** key allows access to the parameters within a list. Some parameters are display-only; others may be altered by the operator. Some parameters only appear in appropriate circumstances – for example, working setpoint does not appear if setpoint ramp rate is Off.

A single press of the scroll key displays the temperature units; further presses reveal the parameters in the current list indicated in the Navigation Diagram.

To return to the Home list at any time, press Page and Scroll together, or wait for 45 seconds.

The **Down** and **Up** keys are used to alter the setpoint or other parameter values.

2.3 Basic Operation

Normally no operator action is required other than entering the setpoint, as the 201 starts to control on being switched on, as described above.

2.4 Altering the Setpoint

With the display at “home”, showing the measured temperature, press Down or Up once to display the setpoint; press again or hold down to adjust it. The display returns to the measured temperature when no key is pressed for 0.5 seconds.

2.5

Stopping and Starting Control

It is possible to stop and start the controller without altering the setpoint. Press Scroll  until the legend m-A (manual/auto) appears. In the 201, manual means “off” and auto means “on”. Press Down  or Up  once to show the current on/off state: mAn for off, and Auto for on. Press  or  to change between manual and auto (off and on) as required.

2.6 Altering the Ramp Rate

It is possible to limit the rate of heating by setting a ramp rate. Press Scroll  until the legend SPrr (SetPoint ramp rate) is displayed. Use Down  or Up  to display and adjust the value.

The ramp rate sets the maximum rate of heating or cooling in degrees per minute. A value of OFF cancels the ramp rate, allowing heating and cooling at the maximum rate. When this feature is in use, there is a “working setpoint” which can be viewed at any time by scrolling to w.SP and pressing  or .

Fig 1 and fig 2 indicate the possible difference between running without and with a ramp-to-setpoint value (depending on the load and the value used).

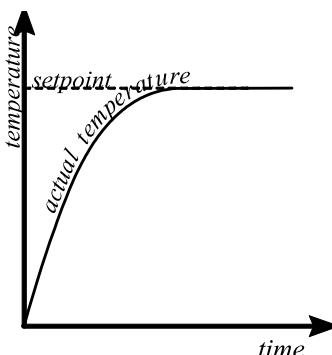


fig 1 - control without ramp-to-setpoint

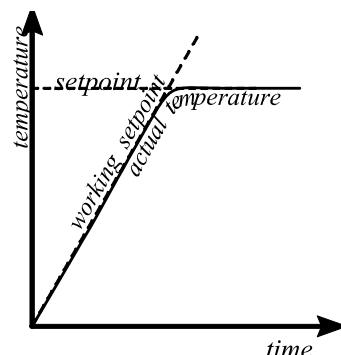


fig 2 - control with ramp-to-setpoint

OVERTEMPERATURE OPTION

This is only fitted when the overtemperature option is ordered. To identify whether it is fitted, observe the controller panel: if it is fitted the overtemperature key and warning light are present.

The overtemperature key must be held depressed continuously while viewing or adjusting the overtemperature controller. If the Overtemperature key is released, the display reverts to the main controller.

With the key pressed the overtemperature setpoint is normally displayed. To alter the value, use Down and Up. To view the measured temperature, press Scroll until PV (process variable) is displayed, then press Down or Up. Keep the overtemperature key depressed during these operations.

When an overtemperature condition is reached, the overtemperature warning light changes from green to flashing red. To “accept” or “reset” this alarm condition, press the Overtemperature key and the Page key together; the warning light changes to continuous red. Once the overtemperature condition is cleared (by the temperature falling), the light changes to green and normal operation resumes.

4 ALTERING THE POWER LIMIT

4.1 Overview

Depending on the furnace or oven model the power limit parameter OP.Hi (Output High) may be accessible or hidden.

For silicon carbide heated furnaces the parameter is accessible to allow for compensation for element ageing (see the appropriate section in the furnace manual). In wire-heated chamber or tube furnaces, reducing the power limit is a convenient method of improving control at low temperatures, as outlined below.

The power limit may be set to zero to permit demonstration of the controls without heating.

In many models the power limit setting depends on the supply voltage; usually the furnace or oven manual contains details: if in doubt, contact Carbolite for advice.

The power limit parameter does not apply to the overtemperature controller, if present.

4.2 Altering the value

Press Page □ until oP (output list) is displayed. Press Scroll ⌂ until OP.Hi (Output High) is displayed. Press Down ▼ or Up ▲ once to display the value of OP.Hi and write down the value. To alter the value, use Down ▼ or Up ▲. Note that setting the value to zero prevents the furnace or oven from heating.

Caution: Do not increase the power limit value to a value above the design level for the oven or furnace model, or to a value above that correctly calculated for Silicon Carbide elements. The heating elements could burn out, or other damage could be caused.

4.3 Control at Low Temperatures

If a product is to be used at temperatures much lower than its design maximum, control stability can often be improved by reducing the power limit. Remember to make a record of the original setting before altering the power limit.

Example: It is desired to run a 1200°C furnace at 300°C. The normal control settings can be expected to cause excessive overshoot as the furnace reaches temperature. If the power limit OP.Hi is normally set to 100%, try a setting of 40%. This should greatly reduce the overshoot. (There is no firm calculation rule to get this example setting of 40% – experiment may be required to achieve a good result. Avoid power limits below about 30% – control accuracy falls off at such levels.)

USER CALIBRATION

The controller is calibrated for life at manufacture against known reference sources, but there may be sensor errors or other system errors. User calibration allows compensation for such errors, and the 201 allows for a user 2-point calibration. This setting is password protected to avoid accidental alteration.

Page to iP, scroll to CAL.P, and use Up ▲ to alter the password. The password is 3. If the correct password is entered, the display shows PASS. Scroll to CAL and use ▼ or ▲ to observe the setting FACT (factory values, as manufactured) or USEr (user values). Change to USEr.

NOTE: before checking the calibration of the controller, or of the complete system, remember to reset the 201 to factory calibration values by setting the CAL.P parameter to FACT.

To enter a user calibration, scroll to each of the following parameters in turn and set the desired values.

Pnt.L low temperature for which an offset is to be entered

OFS.L offset value for the low temperature

Pnt.H high temperature for which an offset is to be entered

OFS.H offset value for the high temperature

Example: the controller reads 3°C low at 400°C, and 5°C low at 1000°C. The parameter values should be Pnt.L=400, OFS.L=3, Pnt.H=1000, OFS.H=5.

Negative or positive values can be entered: if the controller is reading high, negative offsets would be appropriate.

Fig 4 gives a graphical representation of the 2-point calibration.


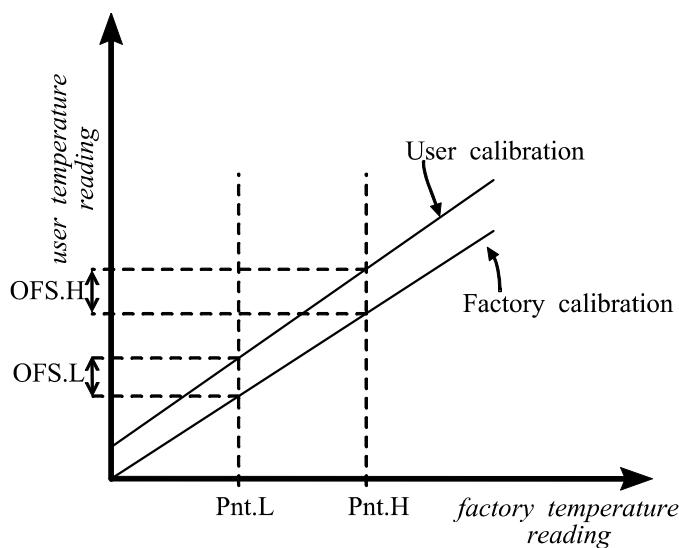


fig 4 - 2-point calibration


NAVIGATION DIAGRAMS

6.1 Main Controller

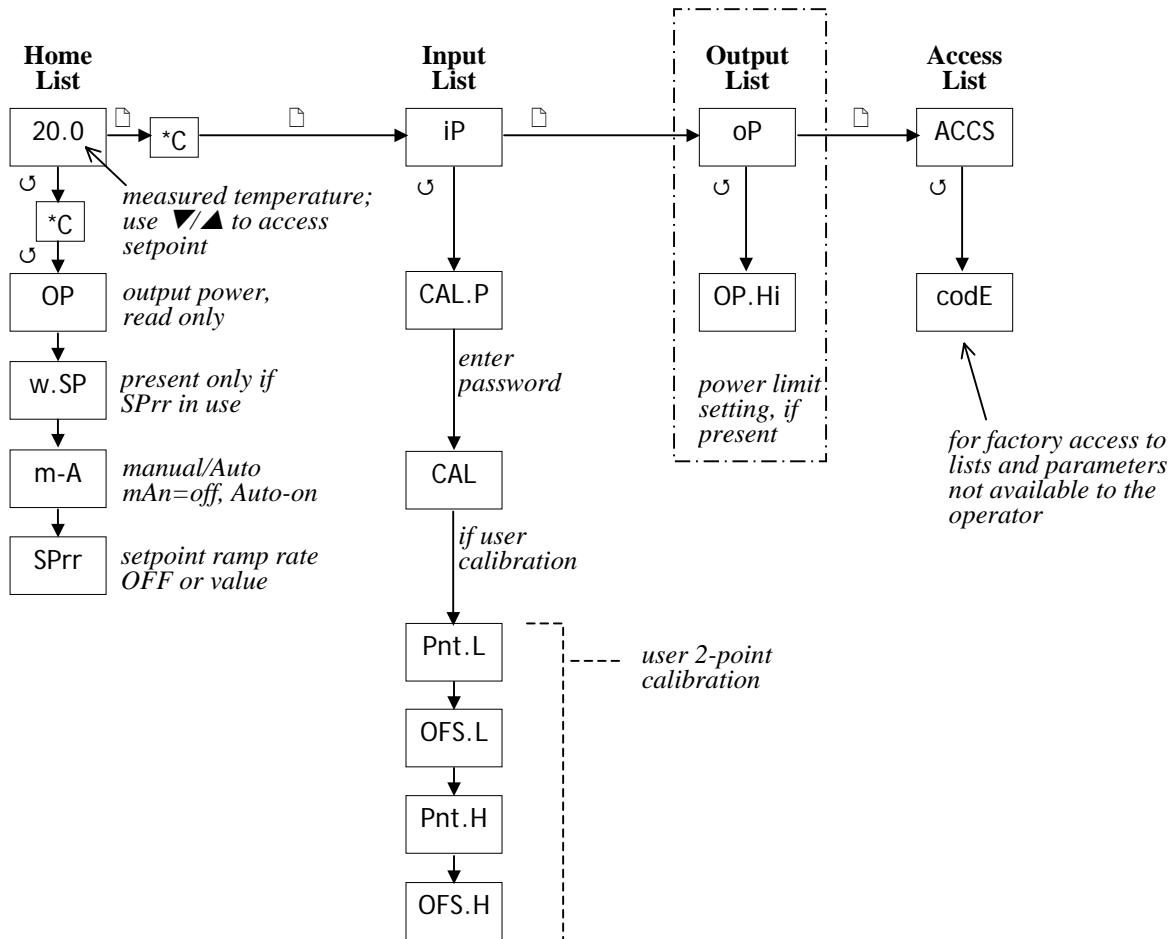

6.2 Overtemperature Controller

Hold the Overtemperature Key to make the parameters in this diagram available.

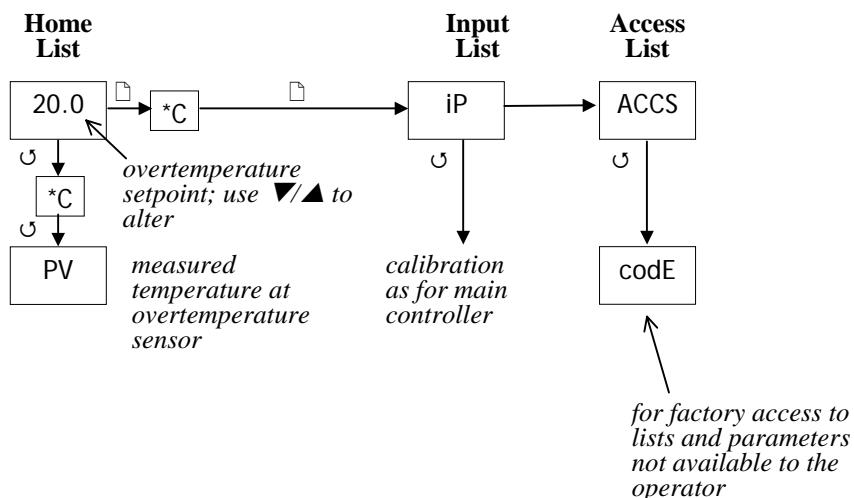



Thank you for reading this data sheet.

For pricing or for further information, please contact us at our UK Office, using the details below.



UK Office
Keison Products,
P.O. Box 2124, Chelmsford, Essex, CM1 3UP, England.
Tel: +44 (0)330 088 0560
Fax: +44 (0)1245 808399
Email: sales@keison.co.uk

Please note - Product designs and specifications are subject to change without notice. The user is responsible for determining the suitability of this product.